

RAYCARE v2026

DICOM Conformance Statement Hitachi Probeat



RayCare

v2026

Declaration of conformity



Complies with Medical Device Regulation (MDR) 2017/745. A copy of the corresponding Declaration of Conformity is available on request.

Safety notices

Warning and caution notices in the user documentation inform about the safe use of the product and must be followed.



WARNING!

A warning notice informs about a risk for bodily harm or death. In most cases, the risk is related to mistreatment of the patient.



CAUTION!

A caution notice informs about a risk for damage to equipment, software or data.

Note: A note provides additional helpful information, tips or reminders.

Copyright

This document contains proprietary information that is protected by copyright. No part of this document may be photocopied, reproduced or translated to another language without prior written consent of RaySearch Laboratories AB (publ).

All Rights Reserved. © 2026, RaySearch Laboratories AB (publ).

Printed material

Hard copies of Instructions for Use and Release Notes related documents are available upon request.

Trademarks

RayAdaptive, RayAnalytics, RayBiology, RayCare, RayCloud, RayCommand, RayData, RayIntelligence, RayMachine, RayOptimizer, RayPACS, RayPlan, RaySearch, RaySearch Laboratories, RayStation, RayStore, RayTreat, RayWorld and the RaySearch Laboratories logotype are trademarks of RaySearch Laboratories AB (publ)*.

Third-party trademarks as used herein are the property of their respective owners, which are not affiliated with RaySearch Laboratories AB (publ).

RaySearch Laboratories AB (publ) including its subsidiaries is hereafter referred to as RaySearch.

* Subject to registration in some markets.

1 OVERVIEW

This document specifies the DICOM interface for the RaySearch Laboratories RayCare treatment management system driver for use with external treatment delivery devices. The driver can export DICOM data associated with a treatment delivery session to the treatment delivery device, as well accept, validate, and store DICOM data related to patient positioning and treatment delivery results received from the treatment delivery device.

1.1 NETWORK SERVICES

SOP Class Name	SOP Class UID	Provider of Service (SCP)	User of Service (SCU)
Transfer			
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	No
RT Beams Delivery Instruction Storage	1.2.840.10008.5.1.4.34.7	Yes	No
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	No
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	No
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	No
Spatial Registration (SRO) Storage	1.2.840.10008.5.1.4.1.1.66.1	Yes	No
Query/Retrieve			
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No
Workflow Management			
Unified Procedure Step - Push SOP Class	1.2.840.10008.5.1.4.34.6.1	Yes	No
Unified Procedure Step - Pull SOP Class	1.2.840.10008.5.1.4.34.6.3	Yes	No
Verification			
Verification SOP Class	1.2.840.10008.1.1	Yes	No

TABLE OF CONTENTS

OVERVIEW	3
NETWORK SERVICES	3
TABLE OF CONTENTS	4
INTRODUCTION	5
REVISION HISTORY	5
AUDIENCE	5
REMARKS	5
TERMS AND DEFINITIONS	5
BASICS OF DICOM COMMUNICATION	6
ABBREVIATIONS	8
REFERENCES	8
NETWORKING	9
IMPLEMENTATION MODEL	9
FUNCTIONAL DEFINITION OF AE	12
NETWORK INTERFACES	17
MEDIA INTERCHANGE	18
TRANSFORMATION OF DICOM TO CDA	19
SUPPORT OF CHARACTER SETS	20
SECURITY	21
SECURITY PROFILES	21
ASSOCIATION LEVEL SECURITY	21
APPLICATION LEVEL SECURITY	21
ANNEXES	22
IOD CONTENTS	22
DATA DICTIONARY OF PRIVATE ATTRIBUTES	50
CODE TERMINOLOGY AND TEMPLATES	51
GRAYSCALE IMAGE CONSISTENCY	51
STANDARD EXTENDED/SPECIALIZED/PRIVATE SOP CLASSES	51
PRIVATE TRANSFER SYNTAXES	51

3 INTRODUCTION

3.1 REVISION HISTORY

3.2 AUDIENCE

This document is written for users that need to understand how the RayCare Hitachi ProBeat driver (hereafter referred to simply as "the driver") will integrate into their healthcare facility. This includes both those responsible for overall imaging network policy and architecture, as well as integrators who need to have a detailed understanding of the DICOM features of the product. This document contains some basic DICOM definitions so that any reader may understand how this product implements DICOM features. However, integrators are expected to fully understand all the DICOM terminology, how the tables in this document relate to the product's functionality, and how that functionality integrates with other devices that support compatible DICOM features.

3.3 REMARKS

The scope of this DICOM Conformance Statement is to facilitate integration between the driver and other DICOM products. The Conformance Statement should be read and understood in conjunction with the DICOM Standard. DICOM by itself does not guarantee interoperability.

- The Conformance Statement does, however, facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.
- This Conformance Statement shall not replace validation with other DICOM equipment to ensure proper exchange of intended information. In fact, it is the user's responsibility to perform the following validation activities:
 - The comparison of Conformance Statements from the driver and other DICOM conformant equipment is the first step towards assessing interconnectivity and interoperability between those systems.
 - Test procedures shall be defined and executed to validate the required level of interoperability with specific DICOM conformant equipment, as established by the healthcare facility.

RaySearch is also active within the IHE-RD. Contact RaySearch for more information regarding adherence to IHE-RD profiles.

3.3.1 DICOM revision

The module tables listed in the last two chapters are based on part 3 of the DICOM-standard edition 2024c. For extra clarity all attributes in the referenced modules have been listed, even the ones that are not used by the driver.

3.4 TERMS AND DEFINITIONS

Informal definitions are provided for the following terms used in this Conformance Statement. The DICOM Standard is the authoritative source for formal definitions of these terms.

Abstract Syntax – the information agreed to be exchanged between applications, generally equivalent to a Service/Object Pair (SOP) Class. Examples: Verification SOP Class, Modality Worklist Information Model Find SOP Class, Computed Radiography Image Storage SOP Class.

Application Entity (AE) – an end point of a DICOM information exchange, including the DICOM network or media interface software; i.e., the software that sends or receives DICOM information objects or messages. A single device may have multiple Application Entities.

Application Entity Title – the externally known name of an Application Entity, used to identify a DICOM application to other DICOM applications on the network.

Application Context – the specification of the type of communication used between Application Entities. Example: DICOM network protocol.

Association – a network communication channel set up between Application Entities.

Attribute – a unit of information in an object definition; a data element identified by a tag. The information may be a complex data structure (Sequence), itself composed of lower level data elements. Examples: Patient ID (0010,0020), Accession Number (0008,0050), Photometric Interpretation (0028,0004), Procedure Code Sequence (0008,1032).

Information Object Definition (IOD) – the specified set of Attributes that comprise a type of data object; does not represent a specific instance of the data object, but rather a class of similar data objects that have the same properties. The Attributes may be specified as Mandatory (Type 1), Required but possibly unknown (Type 2), or Optional (Type 3), and there may be conditions associated with the use of an Attribute (Types 1C and 2C). Examples: MR Image IOD, CT Image IOD, Print Job IOD.

Joint Photographic Experts Group (JPEG) – a set of standardized image compression techniques, available for use by DICOM applications.

Module – a set of Attributes within an Information Object Definition that are logically related to each other. Example: Patient Module includes Patient Name, Patient ID, Patient Birth Date, and Patient Sex.

Negotiation – first phase of Association establishment that allows Application Entities to agree on the types of data to be exchanged and how that data will be encoded.

Protocol Data Unit (PDU) – a packet (piece) of a DICOM message sent across the network. Devices must specify the maximum size packet they can receive for DICOM messages.

Service Class Provider (SCP) – role of an Application Entity that provides a DICOM network service; typically, a server that performs operations requested by another Application Entity (Service Class User). Examples: Picture Archiving and Communication System (image storage SCP, and image query/retrieve SCP), Radiology Information System (modality worklist SCP).

Service Class User (SCU) – role of an Application Entity that uses a DICOM network service; typically, a client. Examples: imaging modality (image storage SCU, and modality worklist SCU), imaging workstation (image query/retrieve SCU)

Service/Object Pair (SOP) Class – the specification of the network or media transfer (service) of a particular type of data (object); the fundamental unit of DICOM interoperability specification. Examples: Ultrasound Image Storage Service, Basic Grayscale Print Management.

Service/Object Pair (SOP) Instance – an information object; a specific occurrence of information exchanged in a SOP Class. Examples: a specific x-ray image.

Tag – a 32-bit identifier for a data element, represented as a pair of four digit hexadecimal numbers, the “group” and the “element”. If the “group” number is odd, the tag is for a private (manufacturer-specific) data element. Examples: {0010,0020} [Patient ID], {07FE,0010} [Pixel Data], {0019,0210} [private data element]

Transfer Syntax – the encoding used for exchange of DICOM information objects and messages. Examples: JPEG compressed (images), little endian explicit value representation.

Unique Identifier (UID) – a globally unique “dotted decimal” string that identifies a specific object or a class of objects; an ISO-8824 Object Identifier. Examples: Study Instance UID, SOP Class UID, SOP Instance UID.

Value Representation (VR) – the format type of an individual DICOM data element, such as text, an integer, a person’s name, or a code. DICOM information objects can be transmitted with either explicit identification of the type of each data element (Explicit VR), or without explicit identification (Implicit VR); with Implicit VR, the receiving application must use a DICOM data dictionary to look up the format of each data element.

3.4.1 RayCare specific terminology

Some terminology used in this Conformance Statement refers to internal concepts used within the application. This section contains a description of these terms.

Beam set – Another name for an RT Plan.

TPS plan – refers to an RT Plan or RT Ion Plan as created by a Treatment Planning System, e.g. RayStation.

Delivery plan – refers to an RT Plan or RT Ion Plan generated by the driver. The plan is generated by taking a TPS plan as input and do some modifications/updates to reflect the current state of the plan in RayCare. Examples of modification are updates to dose reference information for nominal dose tracking and setting of absolute table top positions.

Session – A session is one visit of the patient for treatment, typically from when the patient enters the treatment room to when they leave the treatment room. In practice, an Appointment is scheduled for each Treatment Session.

Fraction delivery – One or more Fraction Deliveries are treated during a Session. A fraction delivery entails either a nominal or continuation treatment for a specific RT Plan.

Fraction number – This is referring to the fraction number in the treatment series. A Treatment series can contain different RT Plans.

Fraction number in beam set – The fraction number within a RT Plan.

3.5 BASICS OF DICOM COMMUNICATION

This section describes terminology used in this Conformance Statement for the non-specialist. This section is not a substitute for training about DICOM, and it makes many simplifications about the meanings of DICOM terms.

Two Application Entities (devices) that want to communicate with each other over a network using DICOM protocol must first perform a network “handshake”. One of the two devices must initiate an Association (a connection to the other device), and ask if specific services, information, and encoding can be supported by the other device (Negotiation).

DICOM specifies a number of network services and types of information objects, each of which is called an Abstract Syntax for the Negotiation. DICOM also specifies a variety of methods for encoding data, denoted Transfer Syntaxes. The Negotiation allows the initiating Application Entity to propose combinations of Abstract Syntax and Transfer Syntax to be used on the Association; these combinations are called Presentation Contexts. The receiving Application Entity accepts the Presentation Contexts it supports.

For each Presentation Context, the Association Negotiation also allows the devices to agree on Roles – which one is the Service Class User (SCU - client) and which is the Service Class Provider (SCP - server). Normally the device initiating the connection is the SCU, i.e., the client system calls the server, but not always.

The Association Negotiation finally enables exchange of maximum network packet (PDU) size, security information, and network service options (called Extended Negotiation information). The Application Entities, having negotiated the Association parameters, may now commence exchanging data. Common data exchanges include queries for worklists and lists of stored images, transfer of image objects and analyses (structured reports), and sending images to film printers. Each exchangeable unit of data is formatted by the sender in accordance with the appropriate Information Object Definition, and sent using the negotiated Transfer Syntax. There is a Default Transfer Syntax that all systems must accept, but it may not be the most efficient for some use cases. Each transfer is explicitly acknowledged by the receiver with a Response Status indicating success, failure, or that query or retrieve operations are still in process.

Two Application Entities may also communicate with each other by exchanging media (such as a CD-R). Since there is no Association Negotiation possible, they both use a Media Application Profile that specifies "pre-negotiated" exchange media format, Abstract Syntax, and Transfer Syntax.

3.6 ABBREVIATIONS

Name	Meaning
AE	Application Entity
AET	Application Entity Title
CT	Computed Tomography
DICOM	Digital Imaging and Communications in Medicine
IHE / IHE-RO	Integrating the Healthcare Enterprise. IHE-RO deals with integrating Radiation Oncology.
IOD	Information Object Definition
JPEG	Joint Photographic Experts Group
MR	Magnetic Resonance Imaging
PACS	Picture Archiving and Communication System
PET	Positron Emission Tomography
RT	Radiotherapy
SCP	Service Class Provider
SCU	Service Class User
SOP	Service-Object Pair
TDD	Treatment Delivery Device
TMS	Treatment Management System
TPS	Treatment Planning System

3.7 REFERENCES

- NEMA PS3 Digital Imaging and Communications in Medicine (DICOM) Standard, available free at <http://medical.nema.org/>

4 NETWORKING

The following diagram illustrates the application data flow between the driver and the specific TDD.

4.1 IMPLEMENTATION MODEL

4.1.1 Application data flow

The diagram displayed in Figure 1 illustrates the application data flow between the driver and the treatment delivery device.

The scenario starts with a C-FIND query for Unified Procedure Steps from the treatment delivery device. The treatment delivery device can then take responsibility for the UPS by setting it to IN PROGRESS. Once the UPS is IN PROGRESS, the driver will only allow requests corresponding to the current session until the session has been completed by the treatment delivery device.

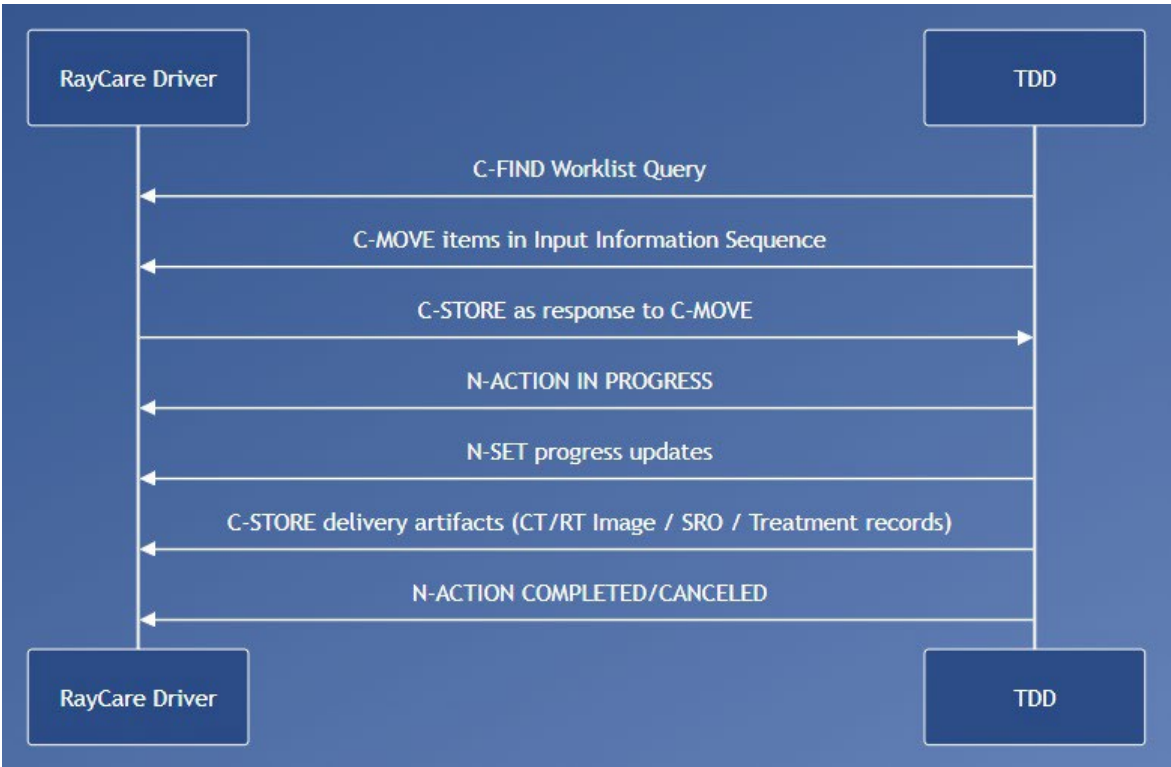


Figure 1

4.1.2 Functional Definition of AEs

4.1.2.1 Functional Definition of the driver Application Entity

The driver Application Entity resides on a workstation that is connected to RayCare. It is a Windows Service which starts up when the workstation on which it resides is started and runs continuously until the workstation is shut down or the service is stopped via services management console. The driver waits for a remote Application Entity to request an association. The driver Application Entity (RAYSEARCH_TX) accepts the association if the proposed context is valid and supported. The driver waits for C-ECHO, C-FIND, N-ACTION, C-STORE and N-SET commands from the remote Application Entity. The associations are maintained by the driver until the remote Application Entity initiates the release process or an abort. The following operations are supported:

Verification

- C-ECHO for connection verification

Unified Procedure Step - Push

- N-ACTION for UPS status changes.
- N-SET for progress update.

Unified Procedure Step - Pull

- C-FIND for worklist query.

RT Beams Delivery Instructions

- C-MOVE for BDIs related to the Unified Procedure Step.

RT Ion Plan

- C-MOVE for RT Ion Plan related to the Unified Procedure Step.

RT Ion Beams Treatment Record

- C-STORE for delivery result.
- C-MOVE for previous delivered results.

CT Image

- C-STORE for setup CT images.
- C-MOVE for planning CT images.

4.1.3 Sequence of Real World Activities

4.1.3.1 Prepare session

Once the session is opened in RayCare Treatment UI the Unified Procedure Step will be created and available for Worklist queries.

4.1.3.2 Session delivery

The driver Application Entity does not control the sequence, but it expects the requests to be sent in a certain order. The different activities and their sequencing are described below.

1. C-FIND to get the worklist that consists of zero or many unified procedure steps
 - Request: *Unified Procedure Step - Pull SOP Class*
 - Response: Zero or more Unified Procedure Steps (UPS)
2. C-MOVE to get delivery plan (RT Ion Plan)
 - Options: can be done before or after the UPS is set to *IN PROGRESS*.
 - Request: *Study Root Query/Retrieve Information Model - MOVE*. The requested instances shall be listed in at least one UPS. The following attributes must be included in the request:
 - Query/Retrieve Level (0008,0052) - Needs to be IMAGE
 - SOP Instance UID (0008,0018)
 - Response: The requested delivery plan instance
3. C-MOVE to get RT Beams Delivery Instruction
 - Options: can be done before or after the UPS is set to *IN PROGRESS*.
 - Request: *Study Root Query/Retrieve Information Model - MOVE*. The requested instances shall be listed in at least one UPS. The following attributes must be included in the request:
 - Query/Retrieve Level (0008,0052) - Needs to be IMAGE
 - SOP Instance UID (0008,0018)
 - Response: The requested RT Beams Delivery Instruction instance
4. C-MOVE to get RT Ion Beams Treatment Record for previous deliveries
 - Options: can be done before or after the UPS is set to *IN PROGRESS*.
 - Request: *Study Root Query/Retrieve Information Model - MOVE*. The requested instances shall be listed in at least one UPS. The following attributes must be included in the request:
 - Query/Retrieve Level (0008,0052) - Needs to be IMAGE
 - SOP Instance UID (0008,0018)
 - Response: The requested Treatment Record
5. C-MOVE to get images referenced in the UPS Input Information Sequence (0040,4021)
 - Options: can be done before or after the UPS is set to *IN PROGRESS*.
 - Request: *Study Root Query/Retrieve Information Model - MOVE*. The requested instances shall be listed in at least one UPS. The following attributes must be included in the request:
 - Query/Retrieve Level (0008,0052) - Needs to be SERIES
 - Series Instance UID (0020,000E)
 - Response: All instances in the requested image series
6. C-MOVE to get other items listed in the UPS Input Information Sequence (0040,4021)
 - Options: can be done before or after the UPS is set to *IN PROGRESS*.
 - Request: *Study Root Query/Retrieve Information Model - MOVE*.
 - Query/Retrieve Level (0008,0052) - Needs to be IMAGE
 - SOP Instance UID (0008,0018)
 - Response: The requested instance
7. N-ACTION to claim UPS and set it to *IN PROGRESS*

- Request: *UPS Push SOPClass*. The following attributes shall be included in the request in addition to the command attributes defined in the DICOM standard:
 - Transaction UID (0008,1195) - stored as a 'Locking UID'. No other actor is allowed to update the UPS if the N-Action request is accepted.
 - Procedure Step State (0074,1000) - shall have value *IN PROGRESS*
 - Response: *UPS Push SOPClass*. If the response status is anything other than successful, it is expected that the TDD does not allow delivery.
 - Transaction UID (0008,1195) - confirmation of the 'Locking UID'
 - Procedure Step State (0074,1000) - confirmation of the current state
- 8. *[Conditional]* If the TDD determines that the delivery can not be performed after an UPS has been set to *IN PROGRESS*, the UPS can be canceled using a N-ACTION command
 - Request: *UPS Push SOPClass*. The following attributes shall be included in the request in addition to the command attributes defined in the DICOM standard:
 - Transaction UID (0008,1195) - Must match 'Locking UID' from when UPS was set to *IN PROGRESS*
 - Procedure Step State (0074,1000) - shall have value *CANCELED*
 - Response: *UPS Push SOPClass*
 - Transaction UID (0008,1195) - confirmation of the 'Locking UID'
 - Procedure Step State (0074,1000) - confirmation of the current state
- 9. N-SET with progress update sent from TDD to driver.
 - At least a N-SET with progress 0 to indicate that work is about to start is required.
 - If delivery completes as intended a N-SET with progress 100 to indicate that work finished is required.
 - If N-SET is sent for UPS not in state *IN PROGRESS*, the driver responds with an error status code.
 - Request: *UPS Push SOPClass*. The following attributes shall be included in the request in addition to the command attributes defined in the DICOM standard:
 - Transaction UID (0008,1195) - Must match 'Locking UID' from when UPS was set to *IN PROGRESS*
 - Procedure Step Progress Information Sequence (0074,1002)
 - Procedure Step Progress (0074,1004) - will be logged in TMS as progress. Does not need to be related to delivered meterset.
 - *Optional*: Procedure Step Progress Description (0074,1006) - will be logged in TMS as progress description.
 - *Optional*: Procedure Step Progress Parameters Sequence (0074,1007) - If an item with concept 'Referenced Beam Number' is included it will be logged in TMS as beam in progress.
 - Response: *UPS Push SOPClass*
 - Transaction UID (0008,1195) - confirmation of 'Locking UID'
 - Procedure Step Progress Information Sequence (0074,1002)
 - Procedure Step Progress (0074,1004) - confirmation of progress.
 - *Optional*: Procedure Step Progress Description (0074,1006) - confirmation of description.
 - *Optional*: Procedure Step Progress Parameters Sequence (0074,1007) - Confirmation of 'Referenced Beam Number'.
- 10. C-STORE of delivery artifacts can be sent at any time. Other delivery artifacts than the ones listed below can be sent to the driver. They will be forwarded to the RayCare PACS but they will not be linked to the session. The following artifacts can be stored and linked to session delivery:
 - CT Image Storage
 - RT Image Storage
 - Spatial Registration Storage
 - RT Ion Beams Treatment Record Storage
- 11. N-ACTION to set UPS as *COMPLETED*
 - Request: *UPS Push SOPClass*. The following attributes shall be included in the request in addition to the command attributes defined in the DICOM standard:
 - Transaction UID (0008,1195) - Must match 'Locking UID' from when UPS was set to *IN PROGRESS*
 - Procedure Step State (0074,1000) - shall have value *COMPLETED*
 - Response: *UPS Push SOPClass*. If the response status is anything other than successful, it is expected that the TDD does not allow delivery.
 - Transaction UID (0008,1195) - confirmation of the 'Locking UID'
 - Procedure Step State (0074,1000) - confirmation of the current state

Note: For all N-ACTION and N-SET commands described above, the UPS-Pull SOPClass is negotiated as the Abstract Syntax, but the UPS-Push SOPClass is used as the Requested SOPClass UID the UPS in all subsequent DIMSE messaging.

4.1.3.3 Manual cancellation

The procedure step can be canceled by the user in the application. Further requests relation to the session will be rejected.

4.1.3.4 Complete session

All sessions, including canceled sessions, needs to be completed by the user in the application before another session can be started.

4.2 FUNCTIONAL DEFINITION OF AE

4.2.1 Driver Application Entity

4.2.1.1 SOP Classes

SOP Class Name	SOP Class UID	Provider of Service (SCP)	User of Service (SCU)
Transfer			
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	No
RT Beams Delivery Instruction Storage	1.2.840.10008.5.1.4.34.7	Yes	No
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	No
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	No
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	No
Spatial Registration (SR0) Storage	1.2.840.10008.5.1.4.1.1.66.1	Yes	No
Query/Retrieve			
Study Root Query/Retrieve Information Model- MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No
Workflow Management			
Unified Procedure Step - Push SOP Class	1.2.840.10008.5.1.4.34.6.1	Yes	No
Unified Procedure Step - Pull SOP Class	1.2.840.10008.5.1.4.34.6.3	Yes	No
Verification			
Verification SOP Class	1.2.840.10008.1.1	Yes	No

4.2.1.2 Association Policies

Not applicable

4.2.1.3 General

The DICOM standard Application context shall be specified.

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.1.4 Number of Associations

Any number of incoming concurrent associations are accepted.

4.2.1.5 Asynchronous Nature

The driver does not support asynchronous communication (multiple outstanding transactions over a single Association).

4.2.1.6 Implementation Identity Information

The implementation for this Application Entity is:

Implementation Class UID	1.2.752.243.2
Implementation Version Name	fo-dicom 5.1.3

4.2.1.7 Association Initiation Policy

The driver initiates associations only as part of C-MOVE sub-operations, where it opens a C-STORE association to the requesting AE to transfer the requested instances.

4.2.1.8 Accepted Transfer Syntaxes

The Transfer Syntaxes accepted for each activity is described in the respective section below. Other Transfer Syntaxes might be supported. For questions about other supported values, please contact RaySearch Laboratories.

4.2.1.9 Activity C-ECHO

4.2.1.9.1 Description and Sequencing of Activities

See C-ECHO in the DICOM standard, PS3.7 Chapter 9 http://dicom.nema.org/medical/dicom/current/output/chtml/part07/chapter_9.html

4.2.1.9.2 Accepted Presentation Context

Abstract Syntax Name	Abstract Syntax UID	Transfer Syntax name	Transfer Syntax UID	Role	Extended Negotiation
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.10 Activity C-FIND

4.2.1.10.1 Description and Sequencing of Activities

See C-FIND in the DICOM standard, PS3.7 Chapter 9 http://dicom.nema.org/medical/dicom/current/output/chtml/part07/chapter_9.html

4.2.1.10.2 Accepted Presentation Context

Abstract Syntax Name	Abstract Syntax UID	Transfer Syntax name	Transfer Syntax UID	Role	Extended Negotiation
Unified Procedure Step - Pull SOP Class	1.2.840.10008.5.1.4.34.6.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.10.3 SOP Specific Conformance for Query SOP Classes - Worklist query

For C-FINDs for Unified Procedure Steps the matching is done as described below.

Attribute Name	Tag	VR	Types of Matching	Comment
Procedure Step State	{0074,1000}	CS	S	The value <i>SCHEDULED</i> is required.
Scheduled Workitem Code Sequence	{0040,4018}	SQ	SQ	A sequence with a single item is optional.
> Code Value	{0008,0100}	SH	S	If set to 121728, then only UPS of type RT Treatment with Internal Verification will be returned. If set to 121726, then only UPS of type RT Treatment QA with Internal Verification will be returned.
Scheduled Station Name Code Sequence	{0040,4025}	SQ	SQ	A sequence with a single item is required.
> Code Value	{0008,0100}	SH	S	The name of the device that the UPS must be assigned to. This needs to match the Device Name that the RayCare Driver is configured for. For QA UPSs this can also match the RayCare Driver's configured Device Name Alias.

Scheduled Procedure Step Start Date and Time	{0040,4005 }	DT	R	The date time is expressed in local driver time unless a Timezone Offset From UTC {0008,0201} is set.
---	-----------------	----	---	--

The table should be read as follows:

Types of matching [See section C.2.2.2 “Attribute Matching” in PS3.4; https://dicom.nema.org/medical/dicom/current/output/chtml/part04/sect_C.2.2.2.htm l):

S - Indicates the identifier attributes uses Single Value Matching.

SQ - Indicates the identifier attributes uses Sequence Matching.

R - Indicates Range Matching.

The returned Query Keys are described in the [Created SOP Instance\[s\]](#) section.

4.2.1.11 Activity C-MOVE

4.2.1.11.1 Description and Sequencing of Activities

See C-MOVE in the DICOM standard, PS3.7 Chapter 9 http://dicom.nema.org/medical/dicom/current/output/chtml/part07/chapter_9.html

4.2.1.11.2 Accepted Presentation Context

Abstract Syntax Name	Abstract Syntax UID	Transfer Syntax name	Transfer Syntax UID	Role	Extended Negotiation
RT Beams Delivery Instruction Storage	1.2.840.10008.5.1.4.34.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Information Model- MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.12 Activity C-STORE

4.2.1.12.1 Description and Sequencing of Activities

The driver accepts storage requests for any artifacts created during a treatment. All received datasets will be archived in the RayCare PACS by the driver. For the SOP Classes listed in the table below, the datasets will also be linked to the current session delivery.

See C-STORE in the DICOM standard, PS3.7 Chapter 9 http://dicom.nema.org/medical/dicom/current/output/chtml/part07/chapter_9.html

4.2.1.12.2 Accepted Presentation Context

Abstract Syntax Name	Abstract Syntax UID	Transfer Syntax name	Transfer Syntax UID	Role	Extended Negotiation
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.123 Status Response

Service Status	Further meaning	Error Code	Reason
Failure	Storage Cannot Understand	Cxxx	Cannot find session or validation failed.
	SOP class not supported	0122	SOP class not supported.
Success	Success	0000	

4.2.1.13 Activity N-ACTION

4.2.1.13.1 Description and Sequencing of Activities

See N-ACTION in the DICOM standard, PS3.7 Chapter 10

https://dicom.nema.org/medical/dicom/current/output/chtml/part07/chapter_10.html

4.2.1.13.2 Accepted Presentation Context

Abstract Syntax Name	Abstract Syntax UID	Transfer Syntax name	Transfer Syntax UID	Role	Extended Negotiation
Unified Procedure Step - Push SOP Class	1.2.840.10008.5.1.4.34.6.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.13.3 SOP Specific Conformance for Status Change

If the Requested SOP Class UID {0000,0003} is *Unified Procedure Step - Push SOP Class*, the Requested SOP Instance UID {0000,1001} matches an existing UPS and Action Type ID {0000,1008} has value "1", the status change is done as described below.

Attribute Name	Tag	VR	Comment
Procedure Step State	{0074,1000}	CS	Either of the values below are supported: • IN PROGRESS • CANCELED • COMPLETED

Transaction UID	{0008,1195}	UI	Must be included in the N-ACTION request when the UPS is set to IN PROGRESS by the TDD. The driver will save the value, and the same value must be used throughout the whole UPS lifecycle to change its state and progress.
-----------------	-------------	----	--

4.2.1.13.4 Status Response

Service Status	Further meaning	Error Code	Reason
Refused	QueryRetrieveUnableToProcess	C000	Unknown SOP Instance UID.
	NoLongerUpdateUps	C300	The UPS may no longer be updated.
	IncorrectTransactionUid	C301	The correct Transaction UID was not provided.
	AlreadyInProgress	C302	The UPS is already IN PROGRESS
	SopInstanceUidDoesNotExist	C307	Specified SOP Instance UID does not exist or is not a UPS instance managed by this SCP
Failure	AlreadyCanceled	B304	The UPS is already in the requested state of CANCELED.
	AlreadyCompleted	B306	The UPS is already in the requested state of COMPLETED.
Success	Success	0000	

4.2.1.14 Activity N-SET

4.2.1.14.1 Description and Sequencing of Activities

See N-SET in the DICOM standard, PS3.7 Chapter 10
https://dicom.nema.org/medical/dicom/current/output/chtml/part07/chapter_10.html

4.2.1.14.2 Accepted Presentation Context

Abstract Syntax Name	Abstract Syntax UID	Transfer Syntax name	Transfer Syntax UID	Role	Extended Negotiation
Unified Procedure Step - Push SOP Class	1.2.840.10008.5.1.4.34.6.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.1.14.3 SOP Specific Conformance for Progress Update

If the Requested SOP Class UID {0000,0003} is *Unified Procedure Step - Push SOP Class* and the Requested SOP Instance UID {0000,1001} matches an existing UPS, the status change is done as described below.

Attribute Name	Tag	VR	Comment
Transaction UID	{0008,1195}	UI	Must match UID set by the TDD and first sent when Procedure Step State is set to <i>IN PROGRESS</i> .
Procedure Step Progress Information Sequence	{0074,1002}	SQ	A single item required in the sequence.
> Procedure Step Progress	{0074,1004}	DS	Value representing the current progress. Values between 0 and 100 expected.
> Procedure Step Progress Description	{0074,1006}	ST	Can optionally be sent. Logged by the driver.
> Procedure Step Progress Parameters Sequence	{0074,1007}	SQ	Can optionally be sent. The driver will log a value representing the 'Referenced Beam Number' concept. For more details see section Usage of Attributes From Received IODs in the Annex.

4.2.1.14.4 Status Response

Service Status	Further meaning	Error Code	Reason
Refused	QueryRetrieveUnableToProcess	C000	Unknown SOP Instance UID.
	NoLongerUpdateUps	C300	The UPS may no longer be updated.
	IncorrectTransactionUid	C301	The correct Transaction UID was not provided.
	SopInstanceUidDoesNotExist	C307	Specified SOP Instance UID does not exist or is not a UPS instance managed by this SCP
Success	Success	0000	

4.3 NETWORK INTERFACES

4.3.1 Physical Network Interface

The application is indifferent to the physical medium over which TCP/IP executes, which is dependent on the underlying operating system and hardware.

4.3.2 Additional protocols

None.

4.3.3 IPv4 and IPv6 Support

The driver supports both IPv4 and IPv6. It does not utilize any of the optional configuration identification or security features of IPv6.

4.3.4 Configuration

All configuration is performed with configuration files stored at the installation location. More information about the configuration can be found in the driver installation instructions.

5 MEDIA INTERCHANGE

Not applicable

6 TRANSFORMATION OF DICOM TO CDA

Not applicable

7 SUPPORT OF CHARACTER SETS

The driver supports the following character sets in addition to the default.

- ISO/IR 192

For instances created by the driver, the possible Specific Character Set values are defined in the [Created SOP Instance\(s\)](#) section.

For use cases where the driver only acts as a proxy for the RayCare PACS, character set handling is done according to the RayCare PACS DICOM Conformance Statement.

8 SECURITY

It is the responsibility of the clinic to ensure that the environment where the driver is running is secure. It is assumed that a secured environment includes at a minimum:

- Firewall or router protections to ensure that only approved external hosts have network access to the driver.
- Firewall and router protections to ensure that the driver only has access to approved external hosts and services.
- Any communication with external hosts and services outside the locally secured environment use appropriate secure network channels (e.g. such as a Virtual Private Network (VPN)).

The driver does support Transport Layer Security (TLS) encryption for DICOM communication. It is the responsibility of the clinic to ensure that the certificates used for TLS encryption are properly managed and updated as needed.

The following applies to the driver's TLS support:

- The port used is configurable.
- Key management is done using the Windows certificate store.
- Supported cipher suites depend on Windows because Secure Channel is used.

8.1 SECURITY PROFILES

No Security Profiles are supported.

8.2 ASSOCIATION LEVEL SECURITY

The driver checks the following values for validation of received Association Open Requests:

- Called AE Title.
- Host address of the remote AE (configurable, can be disabled).
- Network stream follows the encryption configurations.

8.3 APPLICATION LEVEL SECURITY

None supported.

9 ANNEXES

9.1 IOD CONTENTS

9.1.1 Created SOP Instance(s)

9.1.1.1 Secondary Capture Image IOD

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	General Series Module	Yes
Frame of Reference	Frame of Reference Module	No
Equipment	SC Equipment Module	Yes
Acquisition	General Acquisition Module	No
Image	General Image Module	Yes
	Image Pixel Module	Yes
	SC Image Module	No
	SOPCommon Module	Yes

9.1.1.1.1 Patient Module

Values copied from delivery plan

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: • M - Male • F - Female 0 • - Other

9.1.1.1.2 General Study Module

Values copied from delivery plan

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	
Study Date	{0008,0020}	DA	2	
Study Time	{0008,0030}	TM	2	
Referring Physician's Name	{0008,0090}	PN	2	
Study ID	{0020,0010}	SH	2	
Accession Number	{0008,0050}	SH	2	

Study Description	{0008,1030}	LO	3	
-------------------	-------------	----	---	--

9.1.1.1.3 General Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: OT.
Series Instance UID	{0020,000E}	UI	1	
Series Number	{0020,0011}	IS	2	
Series Date	{0008,0021}	DA	3	
Series Time	{0008,0031}	TM	3	
Series Description	{0008,103E}	LO	3	
Operators' Name	{0008,1070}	PN	3	

9.1.1.1.4 SC Equipment Module

Attribute name	Tag	Vr	Type	Comment
Conversion Type	{0008,0064}	CS	1	Supported value: WSD.
Modality	{0008,0060}	CS	3	Supported value: OT.
Secondary Capture Device ID	{0018,1010}	LO	3	Set to driver machine name
Secondary Capture Device Manufacturer	{0018,1016}	LO	3	Supported value: RaySearch Laboratories.
Secondary Capture Device Manufacturer's Model Name	{0018,1018}	LO	3	Supported value: RayCare.
Secondary Capture Device Software Versions	{0018,1019}	LO	3	Will contain current RayCare version

9.1.1.1.5 General Image Module

Attribute name	Tag	Vr	Type	Comment
Instance Number	{0020,0013}	IS	2	

9.1.1.1.6 Image Pixel Module

Attribute name	Tag	Vr	Type	Comment
Samples per Pixel	{0028,0002}	US	1	Always set to '3'.
Photometric Interpretation	{0028,0004}	CS	1	Supported value: RGB.
Rows	{0028,0010}	US	1	
Columns	{0028,0011}	US	1	
Bits Allocated	{0028,0100}	US	1	Always set to '8'
Bits Stored	{0028,0101}	US	1	Always set to '8'
High Bit	{0028,0102}	US	1	Always set to '7'
Pixel Representation	{0028,0103}	US	1	Always set as unsigned
Planar Configuration	{0028,0006}	US	1C	Always set to '0'
Pixel Data	{7FE0,0010}	OB or OW	1C	

9.1.1.1.7 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.7 - Secondary Capture Storage
SOP Instance UID	{0008,0018}	UI	1	
Specific Character Set	{0008,0005}	CS	1C	Supported value: ISO_IR 192.
Instance Creation Date	{0008,0012}	DA	3	
Instance Creation Time	{0008,0013}	TM	3	
Timezone Offset From UTC	{0008,0201}	SH	3	

9.1.1.2 RTTreatmentSummary Record IOD

Not all integrations support this IOD.

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	RT Series Module	Yes
Equipment	General Equipment Module	Yes
Treatment Record	RT General Treatment Record Module	Yes
	RT Treatment Summary Record Module	Yes
	SOP Common Module	Yes

9.1.1.2.1 Patient Module

Values copied from delivery plan

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: - M - Male - F - Female 0 - Other

9.1.1.2.2 General Study Module

Values copied from delivery plan

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	
Study Date	{0008,0020}	DA	2	
Study Time	{0008,0030}	TM	2	
Referring Physician's Name	{0008,0090}	PN	2	

Study ID	{0020,0010}	SH	2	
Accession Number	{0008,0050}	SH	2	
Study Description	{0008,1030}	LO	3	

9.1.1.2.3 RT Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: RTRECORD.
Series Instance UID	{0020,000E}	UI	1	
Series Number	{0020,0011}	IS	2	
Series Date	{0008,0021}	DA	3	Set to local date
Series Time	{0008,0031}	TM	3	Set to local time
Series Description	{0008,103E}	LO	3	
Operators' Name	{0008,1070}	PN	2	

9.1.1.2.4 General Equipment Module

Attribute name	Tag	Vr	Type	Comment
Manufacturer	{0008,0070}	LO	2	Supported value: RaySearch Laboratories.
Station Name	{0008,1010}	SH	3	Set to driver machine name
Manufacturer's Model Name	{0008,1090}	LO	3	Supported value: RayCare.
Device Serial Number	{0018,1000}	LO	3	Always set to '0'
Software Versions	{0018,1020}	LO	3	Will contain current RayCare version

9.1.1.2.5 RT General Treatment Record Module

Attribute name	Tag	Vr	Type	Comment
Instance Number	{0020,0013}	IS	1	Always set to '1'
Treatment Date	{3008,0250}	DA	2	
Treatment Time	{3008,0251}	TM	2	
Referenced RT Plan Sequence	{300C,0002}	SQ	2	Will contain reference to delivery plan
>Referenced SOP Class UID	{0008,1150}	UI	1	
>Referenced SOP Instance UID	{0008,1155}	UI	1	

9.1.1.2.6 RT Treatment Summary Record Module

Attribute name	Tag	Vr	Type	Comment
Current Treatment Status	{3008,0200}	CS	1	Supported value: ON_TREATMENT.
First Treatment Date	{3008,0054}	DA	2	Not set if no previous treatment of the RT Plan
Most Recent Treatment Date	{3008,0056}	DA	2	Not set if no previous treatment of the RT Plan
Fraction Group Summary Sequence	{3008,0220}	SQ	3	Always contains a single item
>Referenced Fraction Group Number	{300C,0022}	IS	3	Always references single Fraction Group of delivery plan.
>Fraction Group Type	{3008,0224}	CS	2	Supported value: EXTERNAL_BEAM.
>Number of Fractions Planned	{300A,0078}	IS	2	Set to number of assigned fractions in RayCare

>Number of Fractions Delivered	{3008,005A}	IS	2	Set to number of delivered fractions (fully delivered or partial) of the referenced RT Plan
>Fraction Status Summary Sequence	{3008,0240}	SQ	3	One item for every delivered fraction (completely delivered or partially delivered) included in sequence
>>Referenced Fraction Number	{3008,0223}	IS	1	
>>Treatment Date	{3008,0250}	DA	2	
>>Treatment Time	{3008,0251}	TM	2	
>>Treatment Termination Status	{3008,002A}	CS	2	Supported values: NORMAL, MACHINE, OPERATOR, UNKNOWN.
Treatment Summary Calculated Dose Reference Sequence	{3008,0050}	SQ	3	One item included for every Dose Reference in the delivery plan
>Referenced Dose Reference Number	{300C,0051}	IS	3	
>Dose Reference Description	{300A,0016}	LO	3	Set to same value as in corresponding RT Plan
>Cumulative Dose to Dose Reference	{3008,0052}	DS	1	Set to contain delivered nominal case dose

9.1.1.2.7 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.481.7 - RT Treatment Summary Record Storage
SOP Instance UID	{0008,0018}	UI	1	
Specific Character Set	{0008,0005}	CS	1C	Supported value: ISO_IR 192.
Instance Creation Date	{0008,0012}	DA	3	
Instance Creation Time	{0008,0013}	TM	3	
Timezone Offset From UTC	{0008,0201}	SH	3	

9.1.1.3 RT Ion Plan IOD

Delivery plan is created based on TPS plan. The attributes below are modified when the delivery plan is created.

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	RT Series Module	Yes
Frame of Reference	Frame of Reference Module	Yes
Equipment	General Equipment Module	Yes
Plan	RT General Plan Module	Yes
	RT Prescription Module	Yes
	RT Ion Tolerance Tables Module	Yes
	RT Patient Setup Module	Yes

	RT Fraction Scheme Module	Yes
	RT Ion Beams Module	Yes
	SOPCommon Module	Yes

9.1.1.3.1 Patient Module

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	Only read. Not updated.
Patient ID	{0010,0020}	LO	2	Only read. Not updated.
Patient's Birth Date	{0010,0030}	DA	2	Only read. Not updated.
Patient's Sex	{0010,0040}	CS	2	Only read. Not updated. Supported values: • M - Male • F - Female • - Other

9.1.1.3.2 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	Only read. Not updated.

9.1.1.3.3 RT Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: RTPLAN.
Series Instance UID	{0020,000E}	UI	1	A new UID is generated where ".200" is appended to the Series Instance UID of the TPS plan.
Series Number	{0020,0011}	IS	2	
Series Date	{0008,0021}	DA	3	
Series Time	{0008,0031}	TM	3	
Series Description	{0008,103E}	LO	3	"Delivery plan" is prepended to the series description of the TPS plan.
Operators' Name	{0008,1070}	PN	2	

9.1.1.3.4 Frame of Reference Module

Attribute name	Tag	Vr	Type	Comment
Frame of Reference UID	{0020,0052}	UI	1	Only read. Not updated.

9.1.1.3.5 General Equipment Module

Attribute name	Tag	Vr	Type	Comment
Software Versions	{0018,1020}	LO	3	

9.1.1.3.6 RT General Plan Module

Attribute name	Tag	Vr	Type	Comment
Treatment Protocols	{300A,0009}	LO	3	Only used for validations

Plan Intent	{300A,000A}	CS	3	For QA sessions the value is set to VERIFICATION. For treatment sessions the value is not modified. Supported values: VERIFICATION, CURATIVE, PALLIATIVE, PROPHYLACTIC, MACHINE_QA, RESEARCH, SERVICE.
Referenced Structure Set Sequence	{300C,0060}	SQ	1C	
>Referenced SOP Instance UID	{0008,1155}	UI	1	Only read. Not updated.
Referenced RT Plan Sequence	{300C,0002}	SQ	3	Contains reference to TPS plan.
>Referenced SOP Class UID	{0008,1150}	UI	1	
>Referenced SOP Instance UID	{0008,1155}	UI	1	
>RT Plan Relationship	{300A,0055}	CS	1	Supported values: PREDECESSOR, VERIFIED_PLAN.

9.1.1.3.7 RT Prescription Module

Attribute name	Tag	Vr	Type	Comment
Dose Reference Sequence	{300A,0010}	SQ	3	
>Dose Reference Number	{300A,0012}	IS	1	
>Dose Reference UID	{300A,0013}	UI	3	
>Dose Reference Description	{300A,0016}	LO	3	Only read. Not updated.
>Dose Reference Type	{300A,0020}	CS	1	Supported values: TARGET, ORGAN_AT_RISK.
>Delivery Maximum Dose	{300A,0023}	DS	3	
>Target Prescription Dose	{300A,0026}	DS	3	Updated with the nominal beam set dose specified in RayCare.
>Target Maximum Dose	{300A,0027}	DS	3	
>Organ at Risk Maximum Dose	{300A,002C}	DS	3	

9.1.1.3.8 RT Ion Tolerance Tables Module

Attribute name	Tag	Vr	Type	Comment
Ion Tolerance Table Sequence	{300A,03A0}	SQ	1	At least one tolerance table must exist. Can either be as defined in TPS plan or as defined in RayCare.
>Tolerance Table Number	{300A,0042}	IS	1	Always set to 1.
>Tolerance Table Label	{300A,0043}	SH	3	
>Gantry Angle Tolerance	{300A,0044}	DS	3	
>Beam Limiting Device Angle Tolerance	{300A,0046}	DS	3	
>Beam Limiting Device Tolerance Sequence	{300A,0048}	SQ	3	
>>RT Beam Limiting Device Type	{300A,00B8}	CS	1	Supported values: X, Y, ASYMX, ASYMY, MLCX, MLCY.
>>Beam Limiting Device Position Tolerance	{300A,004A}	DS	1	
>Patient Support Angle Tolerance	{300A,004C}	DS	3	
>Table Top Vertical Position Tolerance	{300A,0051}	DS	3	
>Table Top Longitudinal Position Tolerance	{300A,0052}	DS	3	

>Table Top Lateral Position Tolerance	[300A,0053]	DS	3	
>Table Top Pitch Angle Tolerance	[300A,004F]	FL	3	
>Table Top Roll Angle Tolerance	[300A,0050]	FL	3	
>Snout Position Tolerance	[300A,004B]	FL	3	
>Head Fixation Angle Tolerance	[300A,0152]	DS	3	
>Chair Head Frame Position Tolerance	[300A,0153]	DS	3	
>Fixation Light Azimuthal Angle Tolerance	[300A,0154]	DS	3	
>Fixation Light Polar Angle Tolerance	[300A,0155]	DS	3	

9.1.1.3.9 RT Patient Setup Module

Attribute name	Tag	Vr	Type	Comment
Patient Setup Sequence	[300A,0180]	SQ	1	
>Patient Setup Number	[300A,0182]	IS	1	Only read. Not updated.

9.1.1.3.10 RT Fraction Scheme Module

Attribute name	Tag	Vr	Type	Comment
Fraction Group Sequence	[300A,0070]	SQ	1	
>Number of Fractions Planned	[300A,0078]	IS	2	
>Referenced Beam Sequence	[300C,0004]	SQ	1C	
>>Referenced Beam Number	[300C,0006]	IS	1	Only read. Not updated.
>>Beam Meterset	[300A,0086]	DS	3	Only read. Not updated.

9.1.1.3.11 RT Ion Beams Module

Attribute name	Tag	Vr	Type	Comment
Ion Beam Sequence	[300A,03A2]	SQ	1	
>Beam Number	[300A,00C0]	IS	1	Only read. Not updated.
>Beam Name	[300A,00C2]	LO	1	Only read. Not updated.
>Primary Dosimeter Unit	[300A,00B3]	CS	1	Only read. Not updated. Supported values: MU, NP.
>Referenced Tolerance Table Number	[300C,00A0]	IS	3	Always set to 1.
>Referenced Patient Setup Number	[300C,006A]	IS	3	Only read. Not updated.
>Referenced Reference Image Sequence	[300C,0042]	SQ	3	Only read. Not updated.
>>Referenced SOP Class UID	[0008,1150]	UI	1	Only read. Not updated.
>>Referenced SOP Instance UID	[0008,1155]	UI	1	Only read. Not updated.
>>Reference Image Number	[300A,00C8]	IS	1	Only read. Not updated.
>Treatment Delivery Type	[300A,00CE]	CS	1	Only read. Not updated. Supported values: TREATMENT, SETUP, OPEN_PORTFILM, TRMT_PORTFILM, CONTINUATION.

>Number of Wedges	{300A,00D0}	IS	1	Only read. Not updated.
>Number of Boli	{300A,00ED}	IS	1	Only read. Not updated.
>Referenced Bolus Sequence	{300C,00B0}	SQ	1C	Only read and displayed in Treat UI. Not updated.
>>Referenced ROI Number	{3006,0084}	IS	1	
>>Bolus ID	{300A,00DC}	SH	3	
>Snout Sequence	{300A,030C}	SQ	3	
>>Snout ID	{300A,030F}	SH	1	Only read. Not updated.
>Applicator Sequence	{300A,0107}	SQ	3	Only read. Not updated.
>>Applicator ID	{300A,0108}	SH	1	Only read. Not updated.
>>Applicator Description	{300A,010A}	LO	3	Only read. Not updated.
>General Accessory Sequence	{300A,0420}	SQ	3	Only read. Not updated.
>>General Accessory ID	{300A,0421}	SH	1	Only read. Not updated.
>>General Accessory Description	{300A,0422}	ST	3	Only read. Not updated.
>>General Accessory Type	{300A,0423}	CS	3	Only read. Not updated. Supported values: GRATICULE, IMAGE_DETECTOR, RETICLE.
>Ion Control Point Sequence	{300A,03A8}	SQ	1	
>>Control Point Index	{300A,0112}	IS	1	Only read. Not updated.
>>Meterset Rate	{300A,035A}	FL	3	Only read. Not updated.
>>Gantry Angle	{300A,011E}	DS	1C	Only read. Not updated.
>>Beam Limiting Device Angle	{300A,0120}	DS	1C	Only read. Not updated.
>>Patient Support Angle	{300A,0122}	DS	1C	Only read. Not updated.
>>Table Top Pitch Angle	{300A,0140}	FL	2C	Only read. Not updated.
>>Table Top Roll Angle	{300A,0144}	FL	2C	Only read. Not updated.
>>Table Top Vertical Position	{300A,0128}	DS	2C	Set to delivery table top position defined in RayCare for the beam. Only set in first control point.
>>Table Top Longitudinal Position	{300A,0129}	DS	2C	Set to delivery tabletop position defined in RayCare for the beam. Only set in first control point.
>>Table Top Lateral Position	{300A,012A}	DS	2C	Set to delivery tabletop position defined in RayCare for the beam. Only set in first control point.
>>Snout Position	{300A,030D}	FL	2C	Only read. Not updated.
>>Isocenter Position	{300A,012C}	DS	2C	Only read. Not updated.

9.1.1.3.12 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Copied from TPS plan
SOP Instance UID	{0008,0018}	UI	1	Treatment: A new UID is generated where ".100" is appended to the SOP Instance UID of the TPS plan. QA: A new UID is generated
Instance Creation Date	{0008,0012}	DA	3	
Instance Creation Time	{0008,0013}	TM	3	

9.1.1.4 RT Beams Delivery Instruction IOD

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	General Series Module	Yes
Equipment	General Equipment Module	Yes
Plan	RT Beams Delivery Instruction Module	Yes
	Common Instance Reference Module	No
	SOPCommon Module	Yes

9.1.1.4.1 Patient Module

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: • M - Male • F - Female • - Other

9.1.1.4.2 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	
Study Date	{0008,0020}	DA	2	
Study Time	{0008,0030}	TM	2	
Referring Physician's Name	{0008,0090}	PN	2	
Study ID	{0020,0010}	SH	2	
Accession Number	{0008,0050}	SH	2	
Study Description	{0008,1030}	LO	3	

9.1.1.4.3 General Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: PLAN.
Series Instance UID	{0020,000E}	UI	1	
Series Number	{0020,0011}	IS	2	
Series Date	{0008,0021}	DA	3	
Series Time	{0008,0031}	TM	3	
Series Description	{0008,103E}	LO	3	

9.1.1.4.4 General Equipment Module

Attribute name	Tag	Vr	Type	Comment
Manufacturer	{0008,0070}	LO	2	Supported value: RaySearch Laboratories.
Station Name	{0008,1010}	SH	3	Set to driver machine name
Manufacturer's Model Name	{0008,1090}	LO	3	Supported value: RayCare.
Device Serial Number	{0018,1000}	LO	3	Always set to '0'
Software Versions	{0018,1020}	LO	3	Contains current RayCare version number

9.1.1.4.5 RT Beams Delivery Instruction Module

Attribute name	Tag	Vr	Type	Comment
Referenced RT Plan Sequence	{300C,0002}	SQ	1	
>Referenced SOP Class UID	{0008,1150}	UI	1	Supported values: 1.2.840.10008.5.1.4.1.1.481.5 - RT Plan Storage 1.2.840.10008.5.1.4.1.1.481.8 - RT Ion Plan Storage
>Referenced SOP Instance UID	{0008,1155}	UI	1	
Beam Task Sequence	{0074,1020}	SQ	1	Will contain references to all beams not already treated in the current fraction.
>Beam Task Type	{0074,1022}	CS	1	Set to TREAT for beams with TreatmentDeliveryType TREATMENT. Otherwise set to VERIFY. Supported values: TREAT, VERIFY.
>Treatment Delivery Type	{300A,00CE}	CS	1	Set based on result {record} from last treatment of beam. Supported values: TREATMENT, CONTINUATION.
>Primary Dosimeter Unit	{300A,00B3}	CS	1C	Supported values: MU, MINUTE, NP.
>Continuation Start Meterset	{0074,0120}	FD	1C	
>Continuation End Meterset	{0074,0121}	FD	1C	
>Current Fraction Number	{3008,0022}	IS	1	Populated with "fraction number in beam set".
>Referenced Beam Number	{300C,0006}	IS	1	
Omitted Beam Task Sequence	{300C,0111}	SQ	3	Will contain references to all beams that has already been treated in the current fraction.
>Referenced Beam Number	{300C,0006}	IS	1	
>Reason for Omission	{300C,0112}	CS	1	Supported value: ALREADY_TREATED.

9.1.1.4.6 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Supported values: 1.2.840.10008.5.1.4.34.7 - TDW-2: RT Beams Delivery Instruction Storage 1.2.840.10008.5.1.4.34.1 - TDW-1: RT Beams Delivery Instruction Storage - Trial (Retired)
SOP Instance UID	{0008,0018}	UI	1	

Specific Character Set	{0008,0005}	CS	1C	Supported value: ISO_IR 192.
Instance Creation Date	{0008,0012}	DA	3	Creation date in local time
Instance Creation Time	{0008,0013}	TM	3	Creation date in local time

9.1.1.5 Unified Procedure Step IOD

This section describes the UPS information returned in the worklist C-FIND queries.

IE	Module	Used
Unified Procedure Step	SOPCommon Module	Yes
	Unified Procedure Step Relationship Module	Yes
	Unified Procedure Step Scheduled Procedure Information Module	Yes
	Unified Procedure Step Progress Information Module	Yes
	Unified Procedure Step Performed Procedure Information Module	No
	Patient Demographic Module	No
	Patient Medical Module	No
	Visit Identification Module	No
	Visit Status Module	No
	Visit Admission Module	No

9.1.1.5.1 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOPClass UID	{0008,0016}	UI	1	Supported values: 1.2.840.10008.5.1.4.34.6.1 - TDW-2: Unified Procedure Step - Push 1.2.840.10008.5.1.4.34.4.1 - TDW-1: Unified Procedure Step - Push SOP Class - Trial (Retired)
SOPInstance UID	{0008,0018}	UI	1	
Specific Character Set	{0008,0005}	CS	1C	Supported value: ISO_IR 192.
Instance Creation Date	{0008,0012}	DA	3	
Instance Creation Time	{0008,0013}	TM	3	
Timezone Offset From UTC	{0008,0201}	SH	3	Only included if part of the request.

9.1.1.5.2 Unified Procedure Step Relationship Module

Information copied from TPS plan.

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN		
Patient ID	{0010,0020}	LO		
Patient's Birth Date	{0010,0030}	DA		

Patient's Sex	{0010,0040}	CS		Supported values: • M - Male • F - Female • - Other
---------------	-------------	----	--	---

9.1.1.5.3 Unified Procedure Step Scheduled Procedure Information Module

Attribute name	Tag	Vr	Type	Comment
Scheduled Procedure Step Priority	{0074,1200}	CS		Supported value: MEDIUM.
Procedure Step Label	{0074,1204}	LO		Contains RayCare session description.
Scheduled Station Name Code Sequence	{0040,4025}	SQ		
>Code Value	{0008,0100}	SH	1C	Contains the device name for the driver.
>Coding Scheme Designator	{0008,0102}	SH	1C	Supported value: 99IHER02018.
>Code Meaning	{0008,0104}	LO	1	Contains the device name for the driver.
Scheduled Procedure Step Start DateTime	{0040,4005}	DT		Treatment: set to appointment start time. QA: set to start of the day
Expected Completion DateTime	{0040,4011}	DT		Treatment: set to appointment end time QA: set to start of the day
Scheduled Workitem Code Sequence	{0040,4018}	SQ		
>Code Value	{0008,0100}	SH	1C	Supported values: • 121726 - RT Treatment with Internal Verification • 121728 - RT Treatment QA with Internal Verification
>Coding Scheme Designator	{0008,0102}	SH	1C	Supported value: DCM.
>Code Meaning	{0008,0104}	LO	1	Supported values: RT Treatment with Internal Verification, RT Treatment QA with Internal Verification.
Scheduled Processing Parameters Sequence	{0074,1210}	SQ		Will always contain four items. One for each of the following concepts: - Treatment Delivery Type - Plan Label - Current Fraction Number - Number of Fractions Planned
>Value Type	{0040,A040}	CS	1	Will use TEXT for concepts "Treatment Delivery Type" and "Plan Label". Will use NUMERIC for concepts "Current Fraction Number" and "Number of Fractions Planned". Supported values: TEXT, NUMERIC.
>Concept Name Code Sequence	{0040,A043}	SQ	1	

>>Code Value	{0008,0100}	SH	1C	Supported values: 121740 - Treatment Delivery Type 2018001 - Plan Label 2018002 - Current Fraction Number 2018003 - Number of Fractions Planned
>>Coding Scheme Designator	{0008,0102}	SH	1C	Supported values: DCM, 99IHER02018.
>>Code Meaning	{0008,0104}	LO	1	Supported values: Treatment Delivery Type, Plan Label, Current Fraction Number, Number of Fractions Planned.
>Text Value	{0040,A160}	UT	1C	For concept "Plan Label" the value will be populated with the RT Plan Label {300A,0002} of the delivery plan. For concept "Treatment Delivery Type" the value will be populated with either of the supported values below. Supported values: - TREATMENT - Used for concept Treatment Delivery Type if the UPS' fraction delivery is a nominal fraction delivery, that is, no previous partial treatment has occurred for this fraction. - CONTINUATION - Used for concept Treatment Delivery Type if the UPS' fraction delivery is a continuation of a nominal fraction delivery, that is, a previous partial treatment has occurred for this fraction
>Numeric Value	{0040,A30A}	DS	1C	For concept "Current Fraction Number" the value will be populated with the "fraction number in beam set". If no treatment session exists the value "0" is set. For concept "Number of Fractions Planned" the value will be populated with the number of planned fractions for the beam set.
>Measurement Units Code Sequence	{0040,08EA}	SQ	1C	
>>Code Value	{0008,0100}	SH	1C	Supported value: 1.
>>Coding Scheme Designator	{0008,0102}	SH	1C	Supported value: UCUM.
>>Code Meaning	{0008,0104}	LO	1	Supported value: no units.
Input Readiness State	{0040,4041}	CS		Supported values: - READY - An UPS has the READY state when its session has been locked in RayCare and the UPS has fully populated its Input Information Sequence and is ready to be treated. - INCOMPLETE - An UPS has the INCOMPLETE state when its session is not yet locked in RayCare, meaning, treatment relevant properties can still be updated. The Input Information Sequence will not be populated with the needed DICOM references.

Input Information Sequence	{0040,4021}	SQ		Will contain references to DICOM data related to this UPS, including - Delivery plan (RT Plan or RT Ion Plan), one item - RT Beams Delivery Instruction, one item - Treatment Records (RT Beams Treatment Record or RT Ion Beams Treatment Record), one item for each previous treatment record in the same fraction for the delivery plan. - RT Treatment Summary Record, one item with the current Treatment Summary Record
>Type of Instances	{0040,E020}	CS	1	Supported value: DICOM.
>Study Instance UID	{0020,000D}	UI	1C	
>Series Instance UID	{0020,000E}	UI	1C	
>Referenced SOP Sequence	{0008,1199}	SQ	1	
>>Referenced SOP Class UID	{0008,1150}	UI	1	Supported values: 1.2.840.10008.5.1.4.1.1.481.5 - Used if delivery plan is RT Plan 1.2.840.10008.5.1.4.1.1.481.8 - Used if delivery plan is RT Ion Plan 1.2.840.10008.5.1.4.34.7 - RT Beams Delivery Instruction Storage 1.2.840.10008.5.1.4.1.1.481.4 - RT Beams Treatment Record Storage 1.2.840.10008.5.1.4.1.1.481.9 - RT Ion Beams Treatment Record Storage
>>Referenced SOP Instance UID	{0008,1155}	UI	1	
>DICOM Retrieval Sequence	{0040,E021}	SQ	1C	
>>Retrieve AE Title	{0008,0054}	AE	1	Contains AE title of the driver.
Study Instance UID	{0020,000D}	UI		

9.1.1.5.4 Unified Procedure Step Progress Information Module

Attribute name	Tag	Vr	Type	Comment
Procedure Step State	{0074,1000}	CS		Supported value: SCHEDULED.

9.1.2 Usage of Attributes From Received IODs

9.1.2.1 CT Image IOD

Storage of CT images created during a session.

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	General Series Module	Yes
Frame of Reference	Frame of Reference Module	No
	Synchronization Module	No
Equipment	General Equipment Module	No
Acquisition	General Acquisition Module	Yes

Image	General Image Module	No
	General Reference Module	Yes
	ImagePlane Module	No
	ImagePixel Module	No
	Contrast/Bolus Module	No
	CT Image Module	Yes
	Multi-energy CT Image Module	No
	SOPCommon Module	Yes

9.1.2.1.1 Patient Module

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: • M - Male • F - Female 0 • - Other

9.1.2.1.2 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	

9.1.2.1.3 General Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: CT.
Series Instance UID	{0020,000E}	UI	1	
Performed Protocol Code Sequence	{0040,0260}	SQ	3	
>Code Value	{0008,0100}	SH	1C	Used for parsing imaging positions from the Leo chair Supported value: • 200000 - Imaging positions from LEO
>Coding Scheme Designator	{0008,0102}	SH	1C	Supported value: 99LeoCancerCare.
>Code Meaning	{0008,0104}	LO	1	Value not read
>Protocol Context Sequence	{0040,0440}	SQ	3	
>>Value Type	{0040,A040}	CS	1	Value not read
>>Concept Name Code Sequence	{0040,A043}	SQ	1	

>>>Code Value	(0008,0100)	SH	1C	Supported values: 100001 - ChairXPosition 100002 - ChairYPosition 100003 - ChairZPosition 300004 - ChairXAngle 300005 - ChairYAngle 300006 - ChairZAngle 200001 - CT TiltAngle
>>>Coding Scheme Designator	(0008,0102)	SH	1C	Supported value: 99LeoCancerCare.
>>>Code Meaning	(0008,0104)	LO	1	Value not read
>>Numeric Value	(0040,A30A)	DS	1C	

9.1.2.14 General Acquisition Module

Attribute name	Tag	Vr	Type	Comment
Acquisition Date	(0008,0022)	DA	3	
Acquisition Time	(0008,0032)	TM	3	

9.1.2.15 General Reference Module

Attribute name	Tag	Vr	Type	Comment
Referenced Instance Sequence	(0008,114A)	SQ	3	
>Referenced SOP Class UID	(0008,1150)	UI	1	Value not read
>Referenced SOP Instance UID	(0008,1155)	UI	1	If reference matches delivery plan, the image will be linked to the session in RayCare.
>Purpose of Reference Code Sequence	(0040,A170)	SQ	1	Value not read

9.1.2.16 CT Image Module

Attribute name	Tag	Vr	Type	Comment
Image Type	(0008,0008)	CS	1	Value not read
Samples per Pixel	(0028,0002)	US	1	Value not read
Photometric Interpretation	(0028,0004)	CS	1	Value not read
Bits Allocated	(0028,0100)	US	1	Value not read
Bits Stored	(0028,0101)	US	1	Value not read
High Bit	(0028,0102)	US	1	Value not read
Rescale Intercept	(0028,1052)	DS	1	Value not read
Rescale Slope	(0028,1053)	DS	1	Value not read
Table Height	(0018,1130)	DS	3	
Patient Support Angle	(300A,0122)	DS	3	
Table Top Lateral Position	(300A,012A)	DS	3	
Table Top Longitudinal Position	(300A,0129)	DS	3	
Table Top Pitch Angle	(300A,0140)	FL	3	
Table Top Roll Angle	(300A,0144)	FL	3	

9.1.2.1.7 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.2.
SOP Instance UID	{0008,0018}	UI	1	

9.1.2.2 RT Image IOD

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	RT Series Module	Yes
Equipment	General Equipment Module	No
Acquisition	General Acquisition Module	No
Image	General Image Module	No
	Image Pixel Module	No
	Contrast/Bolus Module	No
	Cine Module	No
	Multi-frame Module	No
	RT Image Module	Yes
	SOP Common Module	Yes
	Frame Extraction Module	No

9.1.2.2.1 Patient Module

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: • M - Male • F - Female • - Other

9.1.2.2.2 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	

9.1.2.2.3 RT Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: RTIMAGE.
Series Instance UID	{0020,000E}	UI	1	

9.1.2.2.4 RT Image Module

Attribute name	Tag	Vr	Type	Comment
Samples per Pixel	{0028,0002}	US	1	Value not read
Photometric Interpretation	{0028,0004}	CS	1	Value not read
Bits Allocated	{0028,0100}	US	1	Value not read
Bits Stored	{0028,0101}	US	1	Value not read
High Bit	{0028,0102}	US	1	Value not read
Pixel Representation	{0028,0103}	US	1	Value not read
RT Image Label	{3002,0002}	SH	1	Value not read
Image Type	{0008,0008}	CS	1	Only images where the third value (Image Flavor) is PORTAL or RADIOGRAPH are linked to the treatment session in RayCare. Images with any other Image Flavor will still be persisted in RayCare PACS though. Supported values: ORIGINAL, DERIVED, PRIMARY, SECONDARY, DRR, PORTAL, SIMULATOR, RADIOGRAPH, BLANK, FLUENCE, UNKNOWN.
RT Image Plane	{3002,000C}	CS	1	Value not read
Referenced RT Plan Sequence	{300C,0002}	SQ	3	
>Referenced SOP Class UID	{0008,1150}	UI	1	
>Referenced SOP Instance UID	{0008,1155}	UI	1	If value matches delivery plan, the RT Image will be linked to the current session.
Referenced Beam Number	{300C,0006}	IS	3	Read when reporting acquired image position, to RayCare.
Fraction Number	{3002,0029}	IS	3	
Patient Support Angle	{300A,0122}	DS	3	Read when reporting acquired image position, to RayCare.
Table Top Pitch Angle	{300A,0140}	FL	3	Read when reporting acquired image position, to RayCare.
Table Top Roll Angle	{300A,0144}	FL	3	Read when reporting acquired image position, to RayCare.
Table Top Vertical Position	{300A,0128}	DS	3	Read when reporting acquired image position, to RayCare.
Table Top Longitudinal Position	{300A,0129}	DS	3	Read when reporting acquired image position, to RayCare.
Table Top Lateral Position	{300A,012A}	DS	3	Read when reporting acquired image position, to RayCare.

9.1.2.2.5 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOPClass UID	{0008,0016}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.481.1.
SOPInstance UID	{0008,0018}	UI	1	

9.1.2.3 RT Structure Set IOD

IE	Module	Used
Patient	Patient Module	No
Study	General Study Module	No

Series	RT Series Module	No
Equipment	General Equipment Module	No
Structure Set	Structure Set Module	Yes
	ROI Contour Module	Yes
	RT ROI Observations Module	Yes
	SOP Common Module	Yes

9.1.2.3.1 Structure Set Module

Attribute name	Tag	Vr	Type	Comment
Structure Set Label	{3006,0002}	SH	1	Value not read
Structure Set Date	{3006,0008}	DA	2	
Structure Set Time	{3006,0009}	TM	2	
Referenced Frame of Reference Sequence	{3006,0010}	SQ	3	
>Frame of Reference UID	{0020,0052}	UI	1	Only read if Referenced Frame of Reference Sequence contains a single item.
>RT Referenced Study Sequence	{3006,0012}	SQ	3	
>>Referenced SOP Class UID	{0008,1150}	UI	1	Value not read
>>Referenced SOP Instance UID	{0008,1155}	UI	1	Value not read
>>RT Referenced Series Sequence	{3006,0014}	SQ	1	
>>>Series Instance UID	{0020,000E}	UI	1	
>>>Contour Image Sequence	{3006,0016}	SQ	1	
>>>>Referenced SOP Class UID	{0008,1150}	UI	1	Value not read
>>>>Referenced SOP Instance UID	{0008,1155}	UI	1	
Structure Set ROI Sequence	{3006,0020}	SQ	1	Value not read

9.1.2.3.2 ROI Contour Module

Attribute name	Tag	Vr	Type	Comment
ROI Contour Sequence	{3006,0039}	SQ	1	
>Referenced ROI Number	{3006,0084}	IS	1	
>Contour Sequence	{3006,0040}	SQ	3	Only POINT contours are parsed.
>>Contour Geometric Type	{3006,0042}	CS	1	Supported value: POINT.
>>Number of Contour Points	{3006,0046}	IS	1	Value not read
>>Contour Data	{3006,0050}	DS	1	

9.1.2.3.3 RT ROI Observations Module

Attribute name	Tag	Vr	Type	Comment
RT ROI Observations Sequence	{3006,0080}	SQ	1	
>Observation Number	{3006,0082}	IS	1	Value not read
>Referenced ROI Number	{3006,0084}	IS	1	

>RT ROI Interpreted Type	{3006,00A4}	CS	2	Supported values: ACQ_ISOCENTER, INITLASERISO, INITMATCHISO.
>Material ID	{300A,00E1}	SH	3	Used for bolus material

9.1.2.3.4 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Read and stored.
SOP Instance UID	{0008,0018}	UI	1	Read and stored.
Specific Character Set	{0008,0005}	CS	1C	
Instance Creation Date	{0008,0012}	DA	3	
Instance Creation Time	{0008,0013}	TM	3	

9.1.2.4 Spatial Registration IOD

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	General Series Module	Yes
	Spatial Registration Series Module	No
Frame of Reference	Frame of Reference Module	Yes
Equipment	General Equipment Module	No
Spatial Registration	Spatial Registration Module	Yes
	Common Instance Reference Module	Yes
	General Reference Module	Yes
	SOP Common Module	Yes

9.1.2.4.1 Patient Module

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: • M - Male • F - Female • - Other

9.1.2.4.2 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	

9.1.2.4.3 General Series Module

Attribute name	Tag	Vr	Type	Comment
----------------	-----	----	------	---------

Modality	{0008,0060}	CS	1	
Series Instance UID	{0020,000E}	UI	1	

9.1.2.4.4 Frame of Reference Module

Attribute name	Tag	Vr	Type	Comment
Frame of Reference UID	{0020,0052}	UI	1	

9.1.2.4.5 Spatial Registration Module

Attribute name	Tag	Vr	Type	Comment
Content Date	{0008,0023}	DA	1	
Content Time	{0008,0033}	TM	1	
Instance Number	{0020,0013}	IS	1	Value not read
Content Label	{0070,0080}	CS	1	Value not read
Content Description	{0070,0081}	LO	2	If content description matches delivery plan SOP Instance UID, the spatial registration will be linked to the session in RayCare.
Registration Sequence	{0070,0308}	SQ	1	Value not read

9.1.2.4.6 Common Instance Reference Module

The information in this module is used to locate the two image IODs used to create the registration.

Attribute name	Tag	Vr	Type	Comment
Referenced Series Sequence	{0008,1115}	SQ	1C	
>Series Instance UID	{0020,000E}	UI	1	
>Referenced Instance Sequence	{0008,114A}	SQ	1	
>>Referenced SOP Class UID	{0008,1150}	UI	1	
>>Referenced SOP Instance UID	{0008,1155}	UI	1	
Studies Containing Other Referenced Instances Sequence	{0008,1200}	SQ	1C	
>Study Instance UID	{0020,000D}	UI	1	
>Referenced Series Sequence	{0008,1115}	SQ	1	
>>Series Instance UID	{0020,000E}	UI	1	
>>Referenced Instance Sequence	{0008,114A}	SQ	1	
>>>Referenced SOP Class UID	{0008,1150}	UI	1	
>>>Referenced SOP Instance UID	{0008,1155}	UI	1	

9.1.2.4.7 General Reference Module

Attribute name	Tag	Vr	Type	Comment
Referenced Instance Sequence	{0008,114A}	SQ	3	Contains referenced delivery plan for ProBeat
>Referenced SOP Class UID	{0008,1150}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.481.8 - RT Ion Plan Storage

>Referenced SOP Instance UID	{0008,1155}	UI	1	
>Purpose of Reference Code Sequence	{0040,A170}	SQ	1	Value not read

9.1.2.4.8 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.66.1.
SOP Instance UID	{0008,0018}	UI	1	

9.1.2.5 RT Ion Plan IOD

IE	Module	Used
Patient	Patient Module	No
Study	General Study Module	No
Series	RT Series Module	No
Frame of Reference	Frame of Reference Module	No
Equipment	General Equipment Module	No
Plan	RT General Plan Module	Yes
	RT Patient Setup Module	Yes
	RT Fraction Scheme Module	Yes
	RT Ion Beams Module	Yes
	SOP Common Module	No

9.1.2.5.1 RT General Plan Module

Attribute name	Tag	Vr	Type	Comment
RT Plan Label	{300A,0002}	SH	1	Value not read
RT Plan Geometry	{300A,000C}	CS	1	Value not read

9.1.2.5.2 RT Patient Setup Module

Attribute name	Tag	Vr	Type	Comment
Patient Setup Sequence	{300A,0180}	SQ	1	
>Patient Setup Number	{300A,0182}	IS	1	Value not read
>Setup Technique Description	{300A,01B2}	ST	3	

9.1.2.5.3 RT Fraction Scheme Module

Attribute name	Tag	Vr	Type	Comment
Fraction Group Sequence	{300A,0070}	SQ	1	
>Fraction Group Number	{300A,0071}	IS	1	Value not read
>Number of Fractions Planned	{300A,0078}	IS	2	
>Number of Beams	{300A,0080}	IS	1	Value not read
>Number of Brachy Application Setups	{300A,00A0}	IS	1	Value not read

9.1.2.5.4 RT Ion Beams Module

Attribute name	Tag	Vr	Type	Comment
Ion Beam Sequence	[300A,03A2]	SQ	1	
>Beam Number	[300A,00C0]	IS	1	Value not read
>Beam Name	[300A,00C2]	LO	1	Value not read
>Beam Type	[300A,00C4]	CS	1	Value not read
>Radiation Type	[300A,00C6]	CS	1	Value not read
>Scan Mode	[300A,0308]	CS	1	Value not read
>Primary Dosimeter Unit	[300A,00B3]	CS	1	Value not read
>Virtual Source-Axis Distances	[300A,030A]	FL	1	Value not read
>Referenced Reference Image Sequence	[300C,0042]	SQ	3	
>>Referenced SOP Class UID	[0008,1150]	UI	1	Value not read
>>Referenced SOP Instance UID	[0008,1155]	UI	1	
>>Reference Image Number	[300A,00C8]	IS	1	Value not read
>Treatment Delivery Type	[300A,00CE]	CS	1	Value not read
>Number of Wedges	[300A,00D0]	IS	1	Value not read
>Number of Compensators	[300A,00E0]	IS	1	Value not read
>Number of Boli	[300A,00ED]	IS	1	Value not read
>Number of Blocks	[300A,00F0]	IS	1	Value not read
>Number of Range Shifters	[300A,0312]	IS	1	Value not read
>Number of Lateral Spreading Devices	[300A,0330]	IS	1	Value not read
>Number of Range Modulators	[300A,0340]	IS	1	Value not read
>Patient Support Type	[300A,0350]	CS	1	Value not read
>Number of Control Points	[300A,0110]	IS	1	Value not read
>Ion Control Point Sequence	[300A,03A8]	SQ	1	Value not read

9.1.2.6 RT Ion Beams Treatment Record IOD

Storage of Treatment Record created during a session.

IE	Module	Used
Patient	Patient Module	Yes
Study	General Study Module	Yes
Series	RT Series Module	Yes
Equipment	General Equipment Module	No
Treatment Record	RT General Treatment Record Module	Yes
	RT Treatment Machine Record Module	Yes
	RT Ion Beams Session Record Module	Yes
	SOP Common Module	Yes

9.1.2.6.1 Patient Module

Attribute name	Tag	Vr	Type	Comment
Patient's Name	{0010,0010}	PN	2	
Patient ID	{0010,0020}	LO	2	
Patient's Birth Date	{0010,0030}	DA	2	
Patient's Sex	{0010,0040}	CS	2	Supported values: • M - Male • F - Female • - Other

9.1.2.6.2 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	

9.1.2.6.3 RT Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Supported value: RTRECORD.
Series Instance UID	{0020,000E}	UI	1	
Operators' Name	{0008,1070}	PN	2	

9.1.2.6.4 RT General Treatment Record Module

Attribute name	Tag	Vr	Type	Comment
Instance Number	{0020,0013}	IS	1	Value not read
Treatment Date	{3008,0250}	DA	2	Value stored in RayCare.
Treatment Time	{3008,0251}	TM	2	Value stored in RayCare.
Referenced RT Plan Sequence	{300C,0002}	SQ	2	
>Referenced SOP Class UID	{0008,1150}	UI	1	
>Referenced SOP Instance UID	{0008,1155}	UI	1	

9.1.2.6.5 RT Treatment Machine Record Module

Attribute name	Tag	Vr	Type	Comment
Treatment Machine Sequence	{300A,0206}	SQ	1	
>Treatment Machine Name	{300A,00B2}	SH	2	

9.1.2.6.6 RT Ion Beams Session Record Module

Attribute name	Tag	Vr	Type	Comment
Primary Dosimeter Unit	{300A,00B3}	CS	1	Supported values: MU, NP.
Treatment Session Ion Beam Sequence	{3008,0021}	SQ	1	
>Referenced Beam Number	{300C,0006}	IS	1	
>Beam Name	{300A,00C2}	LO	1	
>Beam Description	{300A,00C3}	ST	3	

>Beam Type	{300A,00C4}	CS	1	Value not read
>Radiation Type	{300A,00C6}	CS	1	Value not read
>Scan Mode	{300A,0308}	CS	1	Value not read
>Number of Wedges	{300A,00D0}	IS	1	Value not read
>Number of Compensators	{300A,00E0}	IS	1	Value not read
>Number of Boli	{300A,00ED}	IS	1	Value not read
>Number of Blocks	{300A,00F0}	IS	1	Value not read
>Recorded Snout Sequence	{3008,00F0}	SQ	1C	
>>Snout ID	{300A,030F}	SH	1	
>Applicator Sequence	{300A,0107}	SQ	1C	
>>Applicator ID	{300A,0108}	SH	1	
>>Applicator Type	{300A,0109}	CS	1	Value not read
>>Applicator Description	{300A,010A}	LO	3	
>General Accessory Sequence	{300A,0420}	SQ	3	
>>General Accessory Number	{300A,0424}	IS	1	Value not read
>>General Accessory ID	{300A,0421}	SH	1	
>>General Accessory Description	{300A,0422}	ST	3	
>>General Accessory Type	{300A,0423}	CS	3	Supported values: GRATICULE, IMAGE_DETECTOR, RETICLE.
>Number of Range Shifters	{300A,0312}	IS	1	Value not read
>Number of Lateral Spreading Devices	{300A,0330}	IS	1	Value not read
>Number of Range Modulators	{300A,0340}	IS	1	Value not read
>Patient Support Type	{300A,0350}	CS	1	Value not read
>Current Fraction Number	{3008,0022}	IS	2	
>Treatment Delivery Type	{300A,00CE}	CS	2	Supported values: TREATMENT, CONTINUATION.
>Treatment Termination Status	{3008,002A}	CS	1	Supported values: NORMAL, OPERATOR, MACHINE, UNKNOWN.
>Specified Primary Meterset	{3008,0032}	DS	3	
>Delivered Primary Meterset	{3008,0036}	DS	3	
>Specified Treatment Time	{3008,003A}	DS	3	
>Delivered Treatment Time	{3008,003B}	DS	3	
>Number of Control Points	{300A,0110}	IS	1	Value not read
>Ion Control Point Delivery Sequence	{3008,0041}	SQ	1	
>>Referenced Control Point Index	{300C,00F0}	IS	1	
>>Treatment Control Point Date	{3008,0024}	DA	1	Value stored in RayCare.
>>Treatment Control Point Time	{3008,0025}	TM	1	Value stored in RayCare.
>>Specified Meterset	{3008,0042}	DS	2	

>>Delivered Meterset	{3008,0044}	DS	1	
>>Meterset Rate Delivered	{3008,0046}	FL	3	
>>Nominal Beam Energy	{300A,0114}	DS	1C	
>>Gantry Angle	{300A,011E}	DS	1C	
>>Gantry Rotation Direction	{300A,011F}	CS	1C	Supported values: NONE, CW, CC.
>>Beam Limiting Device Angle	{300A,0120}	DS	1C	
>>Patient Support Angle	{300A,0122}	DS	1C	
>>Table Top Pitch Angle	{300A,0140}	FL	2C	
>>Table Top Roll Angle	{300A,0144}	FL	2C	
>>Table Top Vertical Position	{300A,0128}	DS	2C	
>>Table Top Longitudinal Position	{300A,0129}	DS	2C	
>>Table Top Lateral Position	{300A,012A}	DS	2C	
>>Snout Position	{300A,030D}	FL	2C	
>>Override Sequence	{3008,0060}	SQ	3	
>>>Parameter Sequence Pointer	{3008,0061}	AT	1	Value not read
>>>Override Parameter Pointer	{3008,0062}	AT	1	
>>>Parameter Item Index	{3008,0063}	IS	1	Value not read
>>>Operators' Name	{0008,1070}	PN	2	

9.1.2.6.7 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOPClass UID	{0008,0016}	UI	1	Supported value: 1.2.840.10008.5.1.4.1.1.481.9.
SOPInstance UID	{0008,0018}	UI	1	

9.1.2.7 RT Radiation Set IOD

IE	Module	Used
Patient	Patient Module	No
Study	General Study Module	Yes
Series	General Series Module	Yes
	Enhanced RT Series Module	No
Equipment	General Equipment Module	No
	Enhanced General Equipment Module	No
Frame of Reference	Frame of Reference Module	No
RT Radiation Set	General Reference Module	No
	RT Radiation Set Module	No
	RT Dose Contribution Module	No
	SOP Common Module	Yes
	Common Instance Reference Module	No

	Radiotherapy Common Instance Module	No
--	-------------------------------------	----

9.1.2.7.1 General Study Module

Attribute name	Tag	Vr	Type	Comment
Study Instance UID	{0020,000D}	UI	1	

9.1.2.7.2 General Series Module

Attribute name	Tag	Vr	Type	Comment
Modality	{0008,0060}	CS	1	Value not read
Series Instance UID	{0020,000E}	UI	1	

9.1.2.7.3 SOP Common Module

Attribute name	Tag	Vr	Type	Comment
SOP Class UID	{0008,0016}	UI	1	
SOP Instance UID	{0008,0018}	UI	1	

9.1.2.8 Unified Procedure Step IOD

This section describes how attributes received in N-ACTION and N-SET command are used.

IE	Module	Used
Unified Procedure Step	SOP Common Module	No
	Unified Procedure Step Relationship Module	No
	Unified Procedure Step Scheduled Procedure Information Module	No
	Unified Procedure Step Progress Information Module	Yes
	Unified Procedure Step Performed Procedure Information Module	No
	Patient Demographic Module	No
	Patient Medical Module	No
	Visit Identification Module	No
	Visit Status Module	No
	Visit Admission Module	No

9.1.2.8.1 Unified Procedure Step Progress Information Module

Attribute name	Tag	Vr	Type	Comment
Procedure Step State	{0074,1000}	CS		Supported values: - IN PROGRESS - Set in N-ACTION by TDD - CANCELED - Set in N-ACTION by the TDD when a session is canceled - COMPLETED - Set in N-ACTION by the TDD when a session is completed normally
Procedure Step Progress Information Sequence	{0074,1002}	SQ		Sent in N-SET requests by the TDD.

>Procedure Step Progress	{0074,1004}	DS		Anumerical value in the range between '0' and '100' is supported. Value logged in application.
>Procedure Step Progress Description	{0074,1006}	ST		Optionally a description for the current progress can be supplied. Value logged in application.
>Procedure Step Progress Parameters Sequence	{0074,1007}	SQ		Optionally an item describing the Referenced Beam Number can be read and logged by the application. Other items are ignored.
>>Value Type	{0040,A040}	CS	1	Supported value: NUMERIC.
>>Concept Name Code Sequence	{0040,A043}	SQ	1	
>>>Code Value	{0008,0100}	SH	1C	Supported value: 2018004 - Referenced Beam Number
>>>Coding Scheme Designator	{0008,0102}	SH	1C	Supported value: 99IHER02018.
>>>Code Meaning	{0008,0104}	LO	1	Supported value: Referenced Beam Number.
>>Numeric Value	{0040,A30A}	DS	1C	Integervalue matching a Beam Number from the delivery plan.
Transaction UID	{0008,1195}	UI	3	TDW-2: Must be included in the N-ACTION request when the UPS is set to IN PROGRESS by the TDD. Stored by the driver and need to match all subsequent N-SET and N-ACTION requests related to this specific UPS.

9.1.3 Attribute Mapping

Not applicable

9.1.4 Coerced/Modified Fields

Not applicable

9.2 DATA DICTIONARY OF PRIVATE ATTRIBUTES

All used Private Creators are listed in the table below. Usage of Private Attributes are listed in each module specification.

Attribute name	Tag	VR	VM	Value
HITACHI	{300F,0010}	LO	1	HITACHI
Table Top CT Vertical Position	{300F,1050}	FL	1	
RaySearch Private Creator	{4001,0010}	LO	1	RAYSEARCHLABS 2.0
TomoPlan SOP Instance UID	{4001,102A}	UI	1	
Varian Medical Systems	{3253,0010}	LO	1	Varian Medical Systems VISION 3253
Extended Interface Data	{3253,1000}	OB	1	
Extended Interface Length	{3253,1001}	IS	1	
Extended Interface Format	{3253,1002}	LO	1	
Varian Medical Systems	{3259,0010}	LO	1	Varian Medical Systems VISION 3259
Additional Dose Value Sequence	{3259,1000}	SQ	1	
Actual Session Dose	{3259,1002}	DS	1	

Daily Dose	{3259,1004}	DS	1	
Life Time Total Dose	{3259,1006}	DS	1	
Varian Medical Systems	{3261,0010}	LO	1	Varian Medical Systems VISION 3261
Treatment Session Beam Data	{3261,102A}	OB	1	
Varian Medical Systems	{3265,0010}	LO	1	Varian Medical Systems VISION 3265
Total Number of Fractions	{3265,1000}	SL	1	
Last Treated Fraction	{3265,1001}	SL	1	

9.3 CODE TERMINOLOGY AND TEMPLATES

Not applicable

9.4 GRAYSCALE IMAGE CONSISTENCY

Not applicable

9.5 STANDARD EXTENDED/SPECIALIZED/PRIVATE SOP CLASSES

9.5.1 Standard extended SOP Class

9.5.2 Specialized SOP Class

Not applicable

9.5.3 Private SOP Class

Not applicable

9.6 PRIVATE TRANSFER SYNTAXES

Not applicable



CONTACT INFORMATION



RaySearch Laboratories AB (publ)
Eugeniavägen 18C
SE-113 68 Stockholm
Sweden

Contact details head office

P.O. Box 45169
SE-104 30 Stockholm, Sweden
Phone: +46 8 510 530 00
Fax: +46 8 510 530 30
info@raysearchlabs.com
www.raysearchlabs.com

RaySearch Americas

Phone: +1 347 477 1935

RaySearch China

Phone: +86 137 0111 5932

RaySearch India

E-mail: manish.jaiswal@raysearchlabs.com

RaySearch Singapore

Phone: +65 8181 6082

RaySearch Australia

Phone: +61 411 534 316

RaySearch France

Phone: +33 (0)1 76 53 72 02

RaySearch Japan

Phone: +81 (0)3 44 05 69 02

RaySearch UK

Phone: +44 (0)2039 076791

RaySearch Belgium

Phone: +32 475 36 80 07

RaySearch Germany

Phone: +49 (0)172 7660837

RaySearch Korea

Phone: +82 01 9492 6432